


# DENTIG

Dental X-ray System  
**TWO-IN-ONE**



**HDX WILL**  
EUROPE GmbH

## Panorama

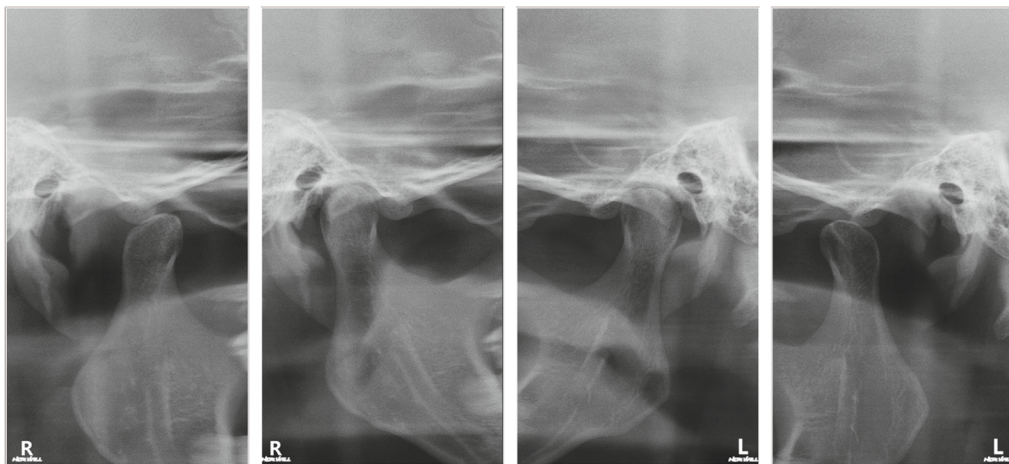


## Cephalometry




## Cut scan time in half

- Less radiation dose
- Less artifacts due to patient movement
- Less patient waiting time

### Panorama

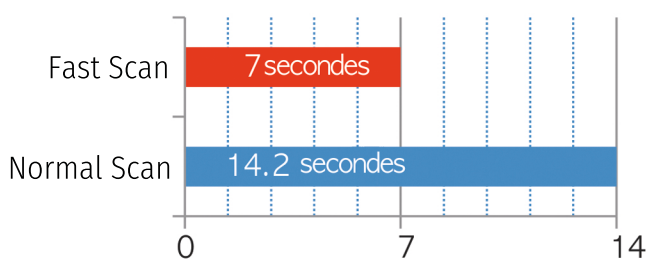

### Cephalometry

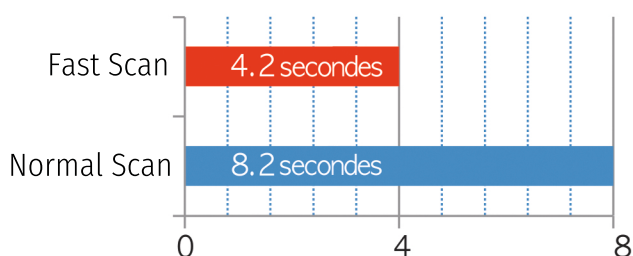

## Technical Specifications

|                   |                                                                                         |
|-------------------|-----------------------------------------------------------------------------------------|
| X-ray Beam        | Cone beam                                                                               |
| kV Range          | 60 kV ~ 90 kV                                                                           |
| mA Range          | 4 mA ~ 10 mA                                                                            |
| Gray Scale        | 16 bits                                                                                 |
| Detector Type     | CMOS                                                                                    |
| Focal spot        | 0.5mm                                                                                   |
| Scan Time         | Panorama : 14.2 s (Normal)/ 7.2 s (Fast)<br>Cephalo : 8.2 s (Normal) / 4.2 s (Fast)     |
| Patient position  | Standing (Wheelchair accessible)                                                        |
| Dimension (W×D×H) | With Cephalo : 1,953 x 1,222 x 2,309 (mm)<br>Without Cephalo : 980 x 1,222 x 2,309 (mm) |
| System Weight     | With Cephalo : 160 kg (tolerance ±10 %)<br>Without Cephalo : 130 kg (tolerance ±10 %)   |

\* Specifications may be updated to improve product performance.

## HDX WILL Europe HQ

Hauptstraße 285, 65760, Eschborn, Germany  
[www.hdxwill.de](http://www.hdxwill.de) / [info@hdxwill.de](mailto:info@hdxwill.de)